
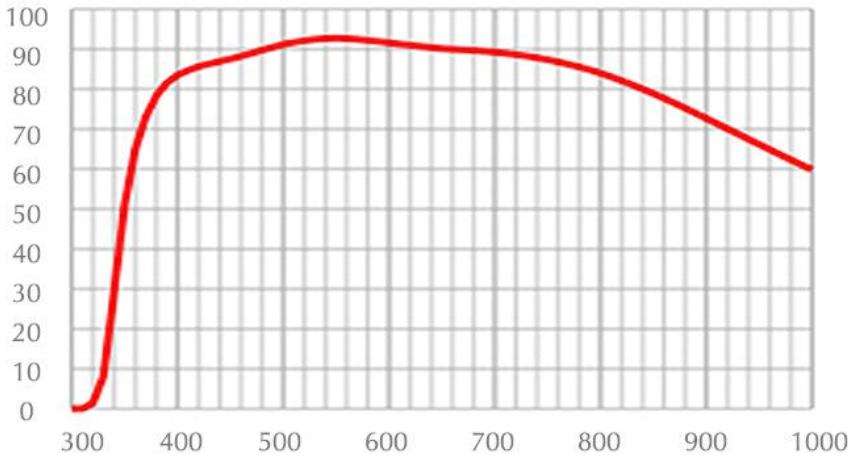
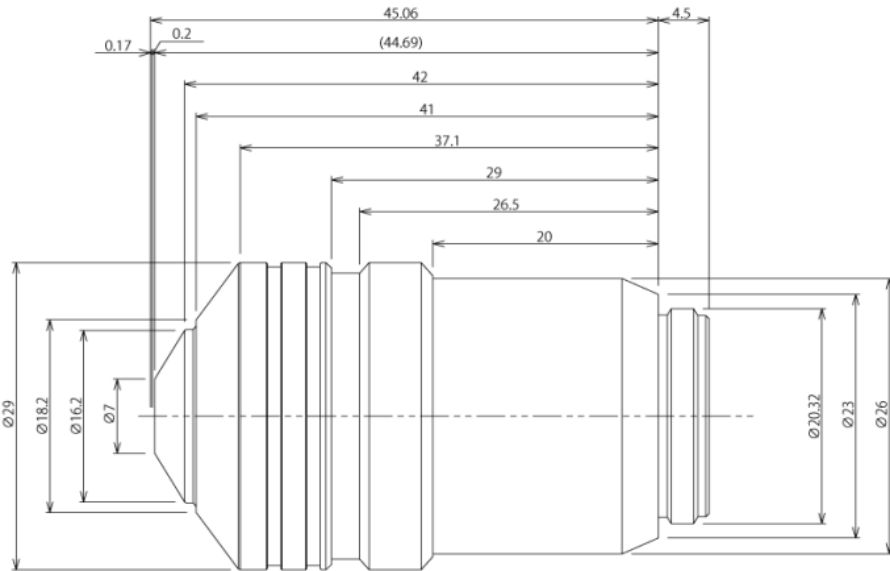


UPLFLN100XOI2

Product Name	UPLFLN100XOI2
Image	 <p style="text-align: center;">Transmittance / Wavelength</p> 
Dimension	
Inquiry	
Web Store	Buy Now
Major Application	Life Science
Magnification [X]	100
Numerical Aperture (NA)	0.60 - 1.30

Last updated: Dec 10 2020

Specifications, design and accessories are subject to change without any notice or obligation on the part of the manufacturer.

UPLFLN100XOI2

Working Distance (WD) [mm]	0.2
Objective Field Number [mm]	26.5
Cover Glass Thickness [mm]	0.17
Immersion Medium	Normal Oil
Spring Loaded	Yes
Correction Collar	N/A
Remarks (Correction Collar)	
Iris	Yes
Correction Level of Chromatic Aberration	Semiapochromat (FL)
Parfocalizing Distance [mm]	45
Back Focal Plane (BFP) Position [mm]	-19.1
Type of Screw Thread	W20.32×0.706 (RMS)
Brightfield (Reflected)	N/A
Brightfield (Transmitted)	Excellent
Darkfield (Reflected)	N/A
Darkfield (Transmitted)	Good
DIC (Reflected)	N/A
DIC (Transmitted)	Excellent
Phase Contrast	N/A
Relief Contrast	N/A
Polarization	Good
Fluorescence (B, G Excitation)	Excellent
UV Fluorescence (at 365 nm)	Excellent
Multiphoton	N/A
TIRF	N/A
IR	N/A
WLI	N/A

Last updated: Dec 10 2020

Specifications, design and accessories are subject to change without any notice or obligation on the part of the manufacturer.

UPLFLN100XOI2

Auto Focus	Yes
Product Number	N1561300
UPC Code	1-U2B5362